


# Patient 1


## ZIKV infection timeline

### After

AD

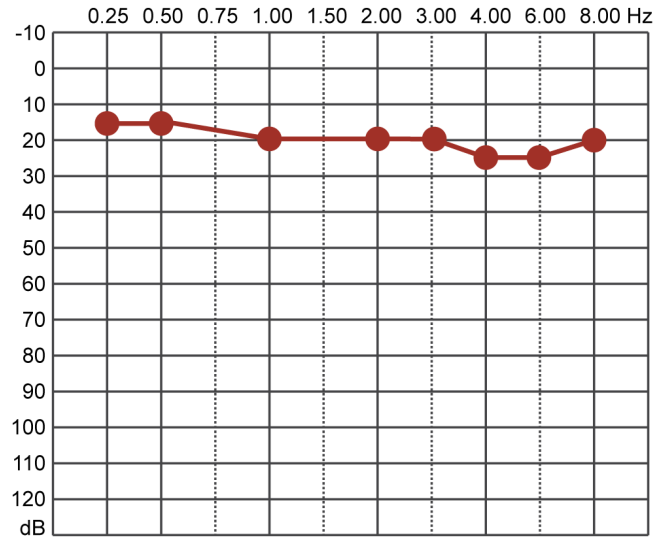

AS

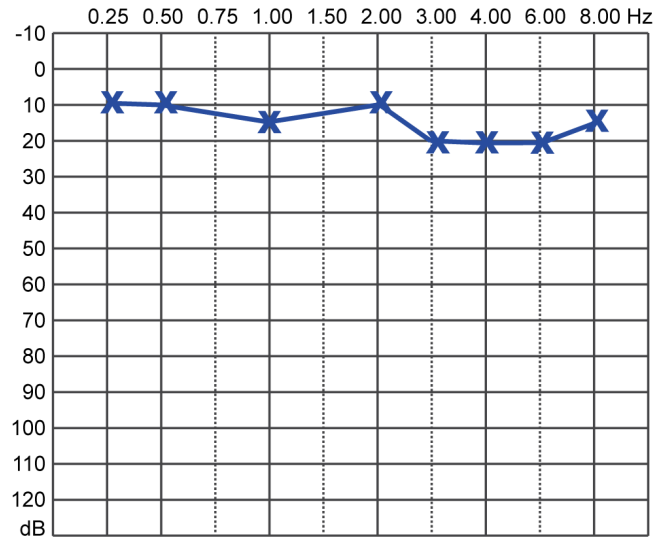

**Supplementary figure 1:** Audiometry exams for ZIKAV-infected patients 1. For the audiometry exams, the frequency in hertz of the test tones is shown on the horizontal axis and sound intensity in decibels is shown on the vertical axis. Red symbols indicate responses for the right ear (AD), and blue indicate responses for the left ear (AS). The “X” and “O” symbols represent responses to air-conducted stimuli. Thresholds of 20 dB or less were considered normal.