



# Optimized broad-range real-time PCR-based method for bacterial screening of platelet concentrates

F. Alexandrino<sup>a</sup> , J. S. Malgarin<sup>a</sup> , M. A. Krieger<sup>a,b</sup> and L. G. Morello<sup>a,b\*</sup>

<sup>a</sup>Instituto de Biologia Molecular do Paraná – IBMP, Curitiba, PR, Brasil

<sup>b</sup>Fundação Oswaldo Cruz, Instituto Carlos Chagas – ICC, Curitiba, PR, Brasil

\*e-mail: [luis.morello@fiocruz.br](mailto:luis.morello@fiocruz.br)

Received: October 11, 2019 – Accepted: March 08, 2020 – Distributed: August 31, 2021  
(With 6 figures)

## Abstract

Bacterial contamination of blood components remains a major challenge in transfusion medicine, particularly, platelet concentrates (PCs) due to the storage conditions that support bacterial proliferation. In this study, we develop a rapid, sensitive and specific real-time PCR protocol for bacterial screening of PCs. An internally controlled real-time PCR-based method was optimized and validated with our proprietary 16S Universal PCR Master Mix (IBMP/Fiocruz), which targets a conserved region of the bacterial 16S rRNA gene. Nonspecific background DNA was completely eliminated by treating the PCR Master Mix with ethidium monoazide (EMA). A lower limit of detection was observed for 10 genome equivalents with an observed Ct value of  $34 \pm 1.07$  in calibration curve generated with 10-fold serial dilutions of *E. coli* DNA. The turnaround time for processing, including microbial DNA purification, was approximately 4 hours. The developed method showed a high sensitivity with no non-specific amplification and a lower time-to-detection than traditional microbiological methods, demonstrating it to be an efficient means of screening pre-transfusion PCs.

**Keywords:** bacterial contamination, real-time PCR, molecular testing, platelet concentrates.

## Otimização de um método baseado em PCR em tempo real para rastreamento de bactérias em concentrados de plaquetas

### Resumo

A contaminação bacteriana dos componentes sanguíneos é um grande desafio na medicina transfusional, principalmente nos concentrados de plaquetas (PCs) devido às condições de armazenamento que favorecem a proliferação bacteriana. Neste estudo, desenvolvemos um protocolo de PCR em tempo real rápido, sensível e específico para a triagem bacteriana de PCs. Um método baseado em PCR em tempo real, controlado internamente, foi otimizado e validado com um Master Mix Universal PCR 16S (IBMP / Fiocruz), que detecta uma região conservada do gene 16S rRNA bacteriano. O background de DNA não específico foi completamente eliminado tratando a PCR Master Mix com monoazida de etídio (EMA). O limite de detecção inferior observado foi de 10 cópias equivalentes do genoma com um valor de Ct  $34 \pm 1,07$ , a curva de calibração foi gerada com diluições seriada de 10 vezes do DNA de *E. coli*. O tempo de processamento, incluindo a purificação microbiana do DNA, foi de aproximadamente 4 horas. O método desenvolvido mostrou alta sensibilidade sem amplificação inespecífica e menor tempo de detecção do que os métodos microbiológicos tradicionais, demonstrando ser um meio eficiente de triagem de PCs pré-transfusionais.

**Palavras-chave:** contaminação bacteriana, PCR em tempo real, teste molecular, concentrado de plaquetas.

### 1. Introduction

Bacterial contamination of blood components is one of the major causes of transfusion-related infection. Despite the implementation of preventive measures, the risk of transfusion-transmitted bacterial infection is still greater than that of transfusion-transmitted viral infection (Brecher et al., 2003). The risk of receiving bacterial-contaminated platelets has been estimated to be 10 to 1,000 times higher than that of receiving platelets contaminated with viruses, such as HIV, HBV, HCV and

HTLV, primarily due to the efficient screening methods used to detect viral pathogens (Blajchman, 2002). In the United States, the residual risk of bacterial contamination is estimated at 1/6,000 for contaminated platelet products and 1/100,000 for septic reactions (Walther-Wenke, 2008).

Transfusion therapies of blood products that are contaminated with bacteria are considered the third most common cause of death reported to the US Food and Drug Administration (FDA), following acute pulmonary

lesions and hemolytic reactions related to transfusion (Razjou et al., 2017). In addition, transfusions of PCs that are contaminated with some type of bacteria can cause serious septic complications to patients.

The primary sources of such contamination include the bacterial skin flora present at puncture regions, asymptomatic bacteremic donors and contamination that occurs during product processing (Palavecino and Yomtovian, 2003; Schrezenmeier et al., 2007). The most frequent bacterial contaminants in PCs are *Staphylococcus* spp., *Streptococcus* spp., *Escherichia coli*, *Bacillus* spp., *Serratia* spp., *Enterobacter* spp., and other organisms (Wagner, 2004).

The prevention or reduction of adverse septic reactions associated with platelets is a major challenge. There have been many advances in technologies and transfusion strategies to reduce the risk of bacterial contamination and sepsis. Some methods can efficiently identify microbial contaminants in PCs, but the time required is an inconvenience, and these methods have low specificity and sensitivity when the initial levels of bacterial contamination are low (Mancini et al., 2010; Ezuki et al., 2007).

Culture methods are capable of detecting as few as one bacterial colony-forming unit (CFU) in a sample and can reliably detect 10 CFU in an inoculated sample without any inhibitors. In general, the BacT/ALERT system is used in Brazil for bacterial screening of PCs, which can detect 1-10 CFU per 5 mL within 24 - 48 hours (Albertoni et al., 2011). The sensitivity of such tests is directly proportional to the bacteria loads and the inoculated volume in a sample. It was previously reported that increasing the sample volume from 4 to 8 mL may significantly increase the detection rate of contaminating bacteria and reduce the risk of transfusion-associated infections (Bruhn et al., 2015). Culture-based techniques are considered the gold standard for detecting bacterial contamination in PCs. However, these methods require large sample volumes and long incubation periods that do not meet all the needs and requirements for a routine assay.

For several years, nucleic acid tests (NAT) have promised to offer more sensitive and faster alternatives to methods based on bacterial growth. These technologies function by rapidly creating copies of DNA from target cells by amplifying the nucleic acid sequences to a detectable level (Mohammadi et al., 2005; Rood et al., 2011).

In a clinical context, real-time PCR is one of the most promising molecular methods for diagnosing infectious diseases with high specificity and sensitivity with a rapid turnaround time using a small sample volume. The sensitivity of real-time PCR screening allows 10-100 CFU/mL to be detected in PCs, depending on the contaminating bacterial species (Esmaili et al., 2017).

Numerous studies have established the 16S rRNA gene as a universal DNA amplification target in a wide range of microorganisms (Wilson et al., 1990; Anderson, 1994; Hendolin et al., 1997; Klausegger et al., 1999). However, the contamination of PCR reagents with microbial DNA is a known problem, particularly when targeting conserved

regions of bacterial genomes using universal primers for broad-range PCR amplification analysis (Garson et al., 2014). Because PCR can amplify low amounts of DNA, co-amplification of trace amounts of contaminating DNA can occur, producing false-positive results. Several different approaches have been described to eliminate or reduce PCR reagent contamination, such as physical, chemical and enzymatic treatments (Hein et al., 2007; Humphrey et al., 2015). The treatment of PCR master mixes with ethidium monoazide (EMA) followed by photoactivation is considered to be the most reliable and effective means of eliminating residual contaminating DNA without compromising the sensitivity of the assay (Hein et al., 2007; Humphrey et al., 2015; Rueckert and Morgan, 2007; Patel et al., 2012; Takahashi et al., 2014).

In this study, we developed a simple, rapid and sensitive broad-range real-time PCR protocol for bacterial screening of PCs that eliminates the problem of co-amplification of contaminating microbial DNA. This protocol will be particularly useful for assaying samples with low levels of contamination and to detect microorganisms that are difficult to grow in vitro or require a long period of incubation.

## 2. Materials and Methods

### 2.1. Real-Time PCR

#### 2.1.1. Design and optimization

A broad-range bacterial PCR detection system targeting a highly conserved region of the 16S rRNA gene was previously described (Yang et al., 2002). Representative 16S rRNA gene sequences for the most common bacterial species causing platelet concentrate contamination were obtained from the GenBank sequence database ([www.ncbi.nlm.nih.gov/genbank/](http://www.ncbi.nlm.nih.gov/genbank/)) (including *Propionibacterium acnes*, *Bacillus cereus*, *Staphylococcus aureus*, *Staphylococcus epidermidis*, *Escherichia coli*, *Serratia marcescens* and *Klebsiella pneumoniae*). The sequences were aligned using MEGA 7 (Kumar et al., 2016). The forward primer sequence was modified to allow *Propionibacterium acnes* to be detected. The optimized oligonucleotide concentrations used were 500 nM of each PCR primer and 250 nM of the hydrolysis probe. The human ribonuclease P gene (encoding RNase P) amplification system was included as internal positive control using 800 nM of each PCR primer and 50 nM of the hydrolysis probe according to a previously described protocol (WHO, 2009). Reactions were performed in a 20 µL final volume using the commercial TaqMan Universal PCR Master Mix (Thermo Fisher Scientific) containing DNA purified from microbial pure culture. A minimum of three reactions were performed for each experiment using the following cycling condition: 95°C for 10 min followed by 40 cycles of 95 °C for 15 sec and 60 °C for 1 min.

#### 2.1.2 Proprietary reaction composition

A proprietary reaction mixture was optimized from a basic PCR reaction buffer (10 mM Tris-HCl (pH 8.8), 50 mM KCl, 0.1% Triton X-100, and 0.1 mM DTT),

supplemented with 1.5 mM MgSO<sub>4</sub>, 0.2 mM dNTPs, 30 nM ROX and 2 units of hot start Taq DNA polymerase. Other salts (MgCl<sub>2</sub> or MgAc) and their concentrations (from 1.5 to 9 mM), as well as additives (BSA, ammonium acetate, potassium glutamate, potassium sulfate and betaine) were also evaluated but did not improve the detection limits or reaction efficiencies. A commercial TaqMan Universal PCR Master Mix (Thermo Fisher Scientific) was used as a reference. The final optimized real-time PCR reaction mixture was produced in our GMP (good manufacturing practices) facility according to quality standards for diagnostics applied to health. Oligonucleotides were synthesized by Integrated DNA Technologies, Inc. (IDT) and were purified by HPLC.

### 2.1.3. Analytical performance

DNA was purified from pure microbial cultures and used to determine the analytical performance of the bacterial 16S rRNA gene detection assay. The purity and quantity of each DNA sample was measured using a DeNovix DS-11+ spectrophotometer (DeNovix Inc., Wilmington, DE, USA). The quantified DNA was diluted 10-fold (10<sup>7</sup> to 10<sup>1</sup> genome equivalents per 5 µL) and 5 µL of each dilution was used as template DNA in PCR reactions to generate the calibration curve. As a control, 10<sup>3</sup> genome equivalents of human DNA was assayed.

### 2.1.4. Removal of contaminant DNA

PCR Master Mix reactions were treated with ethidium monoazide (EMA) as described (Patel et al., 2012) to overcome the contamination of PCR reagents with residual microbial DNA. Briefly, EMA (Sigma-Aldrich) was dissolved in 20% DMSO at a concentration of 10 mg/mL in the dark, after which 50-µL aliquots were stored at -20 °C. Working solutions were prepared fresh on the day of use by dilution in molecular biology grade water (Bioline). The complete PCR Master Mix, including primers and probes, were treated with 1.2 µM EMA and photoactivated on ice with a 500 W halogen light source (Golden) for 5 min at a distance of approximately 20 cm from the tubes. Next, the PCR Master Mix was distributed in the 96-well plate (15 µL), wells were loaded with 5 µL of DNA template or water (no template control, NTC) and real-time PCR was performed on a 7500 Real Time PCR System (Thermo Fisher Scientific). Assays were performed using a minimum of three experimental replicates. Statistical analyses (standard curve, mean ± standard deviation, 95% confidence intervals (CI), coefficient of variation) were calculated using GraphPad Prism v6.0 (Graph Pad Prism Inc., USA).

### 2.2. DNA extraction

Platelet concentrates were processed targeting the enrichment of microbial DNA using a selective lysis approach followed by the disruption of microbial cells with an alkaline solution as described previously (Dobbelaer et al., 2012; Van Meerbergen et al., 2011; Loonen et al., 2013; Trung et al., 2016). Five milliliters of pooled whole blood-derived PCs (1 mL from each of 5 individual donors) was mixed with an equal volume

of selective lysis buffer (500 mM sodium carbonate, 1% Triton X-100, pH 10.5) by inverting the tubes for 30 seconds. The selective lysis step was stopped by the addition of an equal volume of initial sample volume of neutralization buffer (1 M Tris). Intact microbial cells were then concentrated by centrifuging the suspension for 15 minutes at 2,791 xg. Pellets were resuspended in 5 mL of washing buffer (1X phosphate buffered saline - PBS) and then centrifuged for 15 minutes at maximum speed. The resulting pellets were then resuspended in 200 µL of alkaline lysis buffer (200 mM NaOH and 0.5% SDS) and incubated for 10 minutes at 95 °C in a thermomixer set at 1,000 rpm. Finally, 20 µL of neutralization buffer (1 M Citric Acid Solution) was added and the microbial DNA was purified using a QIAamp Blood Mini kit (QIAGEN) according to the manufacturer's protocol.

## 3. Results


### 3.1. Primers and probe design

We evaluated primers and probes described in literature that were primarily developed for universal/pan-bacterial PCR detection. A bioinformatics analysis was performed by aligning 16S rRNA gene sequences of the major bacteria that contaminate platelet concentrates and cause bloodstream infections. A set of universal oligonucleotides specific for the conserved 16S rRNA gene is displayed in Figure 1, showing the P891F-modified primer designed in this study to incorporate the *P. acnes* target sequence.


For primers and probe evaluations, PCR assays were performed with commercial TaqMan Universal PCR Master Mix (Thermo Fisher Scientific). Amplification efficiencies obtained with the forward reference primer (P891F) were compared to the newly designed primer (P891F-modified) using DNA that was purified from pure cultures of *P. acnes* or *E. coli*. The results show that the P891F-modified primer is slightly more efficient than P891F for *P. acnes* DNA amplification (Figure 2A). No difference between the two primers was observed when *E. coli* DNA was used as a template (Figure 2B).

### 3.2. Real-time PCR optimization

We evaluated the effect of several PCR cofactors on the amplification efficiencies of the bacterial 16S rRNA gene in the presence of human genomic DNA. The best experimental optimized condition was named 16S Universal PCR Master Mix (IBMP/Fiocruz) and was compared to the TaqMan Universal PCR Master Mix (Thermo Fisher Scientific) for PCR amplification efficiency. The results show a more efficient reaction with the optimized IBMP/Fiocruz proprietary Master Mix formulation, especially with low quantities of target DNA (Figure 3). As the target quantity decreased, the reaction curve generated with our 16S Universal PCR Master Mix shift to the left compared to the commercial TaqMan Universal PCR Master Mix, presenting lower Ct values (Figure 3A). The human RNase P-encoding gene was amplified in each reaction as an internal control (Figure 3B).

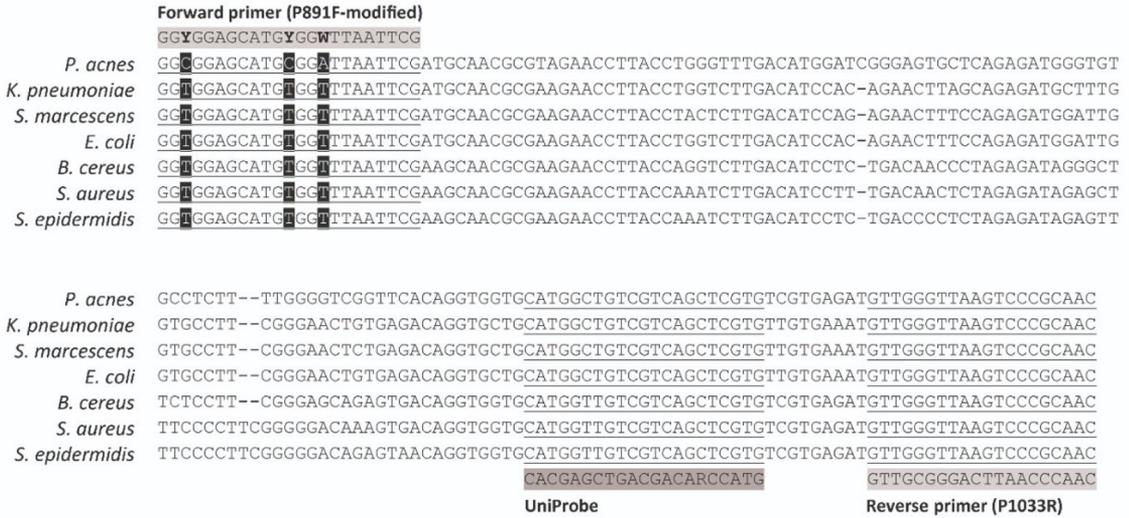

**Figure 1.** Representative nucleotide sequence alignment of the bacterial 16S rRNA gene PCR target. Primers and probes are depicted in the picture. *Propionibacterium acnes* (accession number AB108484), *Klebsiella pneumoniae* (accession number NC\_009648), *Serratia marcescens* (accession number NC\_005211), *Escherichia coli* (accession number AE005174), *Bacillus cereus* (accession number AP007209), *Staphylococcus aureus* (accession number AP017922) and *Staphylococcus epidermidis* (accession number NC\_002976). Sequences were obtained from the GenBank database.

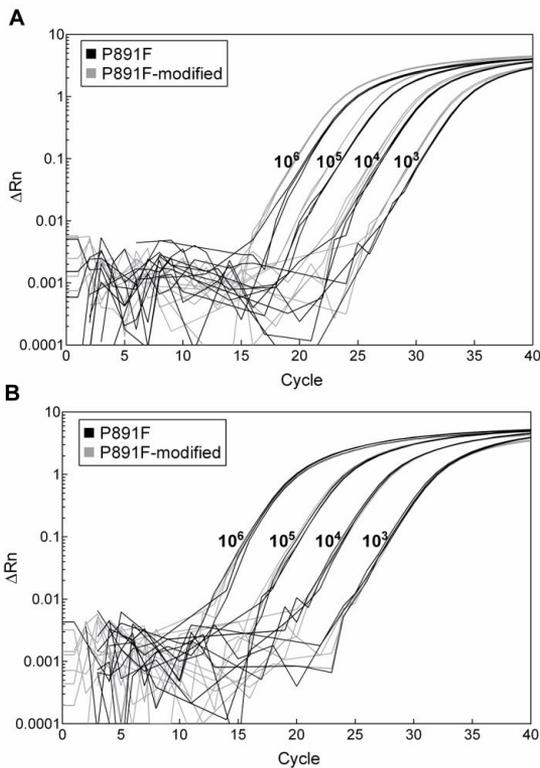

**Figure 2.** Comparison of bacterial 16S rRNA gene amplification efficiencies using the primers P891F (black line) and P891F-modified (gray line). The results were obtained using 10-fold serial dilutions containing 10<sup>6</sup> to 10<sup>3</sup> genome equivalents per reaction. (A) *P. acnes* DNA. (B) *E. coli* DNA.


### 3.3. Analytical sensitivity test

Using a 10-fold dilution calibration curve covering a range of 10<sup>7</sup> to 10<sup>1</sup> genome equivalents per reaction, a linear dynamic range was established with a strong linear correlation (R<sup>2</sup> = 0.999) (Figure 4A). The limit of detection (LoD) of the bacterial 16S rRNA gene, concomitant with the amplification of the human RNase P-encoding gene in duplex reactions, was calculated from the lower concentration with a 95% rate of detection. The LoD was set at 10 bacterial genome equivalents with a Ct value of 34±1.07. GraphPad Prism was set the cut-off value with two standard deviations above the lower LoD detected (95% CI), so the Ct values > 36.19 indicating a negative result.

### 3.4. PCR Master Mix decontamination via EMA treatment

First, the analytical sensitivity of the assay untreated or treated with EMA was evaluated with a 10-fold serial dilution of bacterial DNA from 10<sup>5</sup> to 10<sup>1</sup> genome equivalents per reaction. The untreated and treated with 1.2 μM EMA show equivalent amplification profiles as observed in Figure 4B. No significant difference between the conditions was observed when analyzing the amplification yield or sensitivity of the assay.

Next, the 16S Universal PCR Master Mix that was untreated or treated with 1.2 μM EMA was evaluated for non-specific amplification in no template control reactions (NTC). Each condition was analyzed using 48 replicates in the same 96-well plate. As show in the Figure 5, no amplification was observed using the Master Mix treated

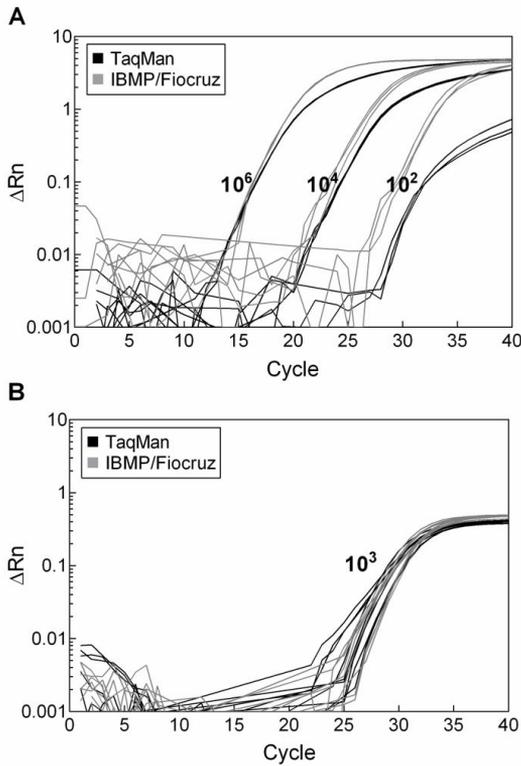


**Figure 3.** Comparison of bacterial 16S gene amplification with 16S Universal PCR Master Mix - IBMP/Fiocruz (grey line) and TaqMan Universal PCR Master Mix - Thermo Fisher Scientific (black line). (A) Amplification plot obtained with a known concentration of *E. coli* DNA ( $10^6$ ,  $10^4$  and  $10^2$  genome equivalents per reaction) in the presence of  $10^3$  copies of human genomic DNA per reaction. (B) Amplification of the human RNase P-encoding gene.


with EMA, while the untreated Master Mix presented non-specific amplification signals with a minimum Ct of 35.45. The results showed a significant difference between untreated and treated Master Mix conditions ( $p = 0.0001$ ) (Fisher, 1956).

### 3.5. Routine platelet screening

This study was performed with PCs from HEMEPAR (Center of Hematology and Haemotherapy of Paraná, Curitiba, Brazil) and was approved by the Institutional Review Board of Hospital do Trabalhador/SES/PR (IRB# 51711815.0.0000.5225). The 16S PCR-based method to screen platelet concentrates for bacteria was evaluated in routine samples undertaken at 24 hours after donation. A total of 250 PCs that were considered negative for bacterial contamination, according to standard protocol applied in the HEMEPAR routine, were analyzed in pools containing five PCs each sample, resulting in 50 samples. The samples were processed on 12 consecutive working days, the results of which are show in Figure 6. A Ct distribution above 37 was observed for the 50 samples assayed, considering that all samples were negative for bacterial contamination.

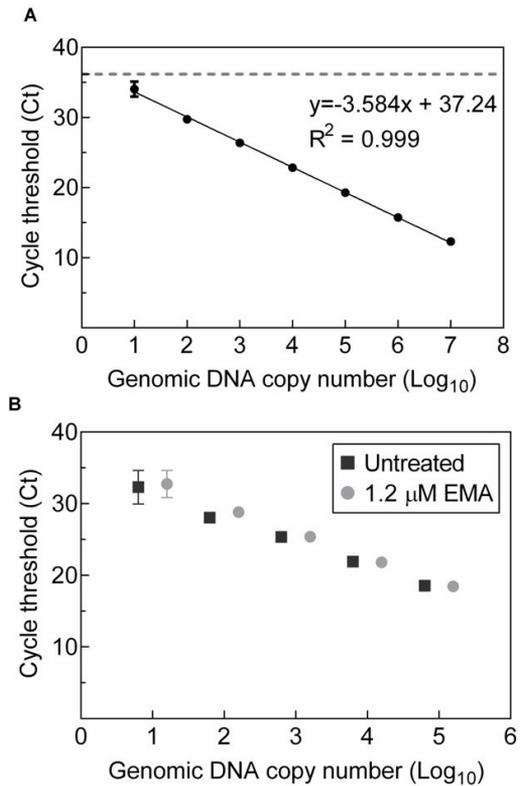

**Figure 4.** Calibration curve generated with 10-fold serial dilutions of *E. coli* DNA. (A) The calibration curve containing  $10^7$  to  $10^1$  genome equivalents per reaction. The assay showed a strong linear dynamic range over 6  $\log_{10}$  concentrations with  $R^2 = 0.999$ . The mean reaction efficiency was 90% with a slope of -3.584 and a y-intercept at 37.24. Dashed line represents the cut-off value (Ct 36.10). The graph was generated using six experimental replicates. (B) Comparison of linear regression of the threshold cycles (Ct) to detect the *E. coli* 16S rRNA gene with PCR Master Mix that was untreated (black square) or treated (grey circle) with ethidium monoazide (EMA). The calibration curve was generated using 10-fold serial dilutions containing  $10^5$  to  $10^1$  genome equivalents per reaction. Paired t-test:  $P > 0.05$  (0.2909).

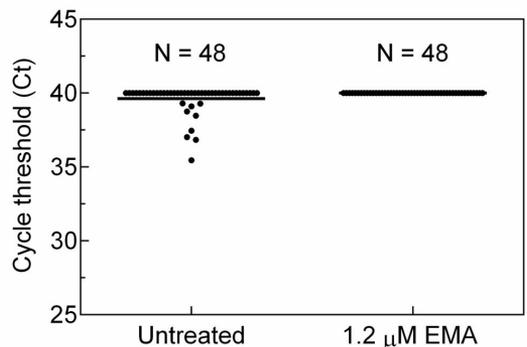

**Figure 5.** Evaluation of non-specific bacterial 16S rRNA gene amplification in no template control (NTC) reactions using PCR Master Mix that was untreated or treated with ethidium monoazide (EMA).



some samples crossed the threshold before 40 cycles with a lower detection point above the established cut-off. These negative results were expected, since approximately 1 in 1,000 to 3,000 platelets units may be contaminated with bacteria (Blajchman et al., 2005; Palavecino et al., 2006; Das et al., 2015).

Molecular techniques can provide information regarding blood contamination during collection or processing and can be implemented in blood banks as a routine screening test to reduce and prevent the risk of transfusion-transmitted bacterial infections. Additionally, this information can be valuable from a statistical and epidemiological point of view, as it could be an opportunity to gain knowledge regarding the contamination detection sources (Mohammadi et al., 2006).

In conclusion, the broad-range real-time PCR-based method described in this study may be used to screen for bacteria in pre-transfusion platelet concentrates. Furthermore, real-time PCR can be integrated into automated sample processing platforms to allow for complete automation of the process, meeting the requirements for blood components screening in blood centers.

## Acknowledgements

We thank Analia Maria Breckenfeld Machado and Adriana Nascimento de Araujo from HEMEPAR for providing routine platelet concentrate samples. This work was supported by the Fundação Oswaldo Cruz.

## References

- ALBERTONI, G., ANDRADE, S.S., ARAUJO, P.R.B., CARVALHO, F.O., GIRÃO, M.J. and BARRETO, J.A., 2011. Evaluation of two detection methods of microorganisms in platelet concentrates. *Transfusion Medicine (Oxford, England)*, vol. 21, no. 6, pp. 408-416. <http://dx.doi.org/10.1111/j.1365-3148.2011.01105.x>. PMID:21895809.
- ANDERSON, B., 1994. Broad-range polymerase chain reaction for detection and identification of bacteria. *The Journal of the Florida Medical Association*, vol. 81, no. 12, pp. 835-837. PMID:7532205.
- ARMBRUSTER, D.A., TILLMAN, M.D. and HUBBS, L.M., 1994. Limit of detection (LOD)/limit of quantification (LOQ): comparison of the empirical and the statistical methods exemplified with GC-MS assays of abused drugs. *Clinical Chemistry*, vol. 40, no. 7, pp. 1233-1238. <http://dx.doi.org/10.1093/clinchem/40.7.1233>. PMID:8013092.
- BENJAMIN, R.J. and WAGNER, S.J., 2007. The residual risk of sepsis: modelling the effect of concentration on bacterial detection in two-bottle culture systems and an estimation of false negative culture rates. *Transfusion*, vol. 47, no. 8, pp. 1381-1389. <http://dx.doi.org/10.1111/j.1537-2995.2007.01326.x>. PMID:17655581.
- BLAJCHMAN, M.A., 2002. Incidence and significance of the bacterial contamination of blood components. *Developmental Biology*, vol. 108, pp. 59-67. PMID:12220143.
- BLAJCHMAN, M.A., BECKERS, E.A., DICKMEISS, E., LIN, L., MOORE, G. and MUYLLE, L., 2005. Bacterial detection of platelets: current problems and possible resolutions. *Transfusion Medicine Reviews*, vol. 19, no. 4, pp. 259-272. <http://dx.doi.org/10.1016/j.tmr.2005.05.002>. PMID:16214015.
- BLAJCHMAN, M.A., GOLDMAN, M. and BAEZA, F., 2004. Improving the bacteriological safety of platelet transfusions. *Transfusion Medicine Reviews*, vol. 18, no. 1, pp. 11-24. <http://dx.doi.org/10.1016/j.tmr.2003.10.002>. PMID:14689374.
- BRECHER, M.E., HAY, S.N. and ROTHENBERG, S.J., 2003. Monitoring of apheresis platelet bacterial contamination with an automated liquid culture system: a university experience. *Transfusion*, vol. 43, no. 7, pp. 974-978. <http://dx.doi.org/10.1046/j.1537-2995.2003.00438.x>. PMID:12823759.
- BRUHN, R., CUSTER, B., VANDERPOOL, S., TOWNSEND, M., KAMEL, H. and TOMASULO, P., 2015. Impact of increasing sample volume from 4 ml to 8 ml on bacterial detection rates in apheresis platelets: a metaanalysis. *Vox Sanguinis*, vol. 108, no. 3, pp. 318-320. <http://dx.doi.org/10.1111/vox.12225>. PMID:25556667.
- BURNS, M. and VALDIVIA, H., 2008. Modelling the limit of detection in real-time quantitative PCR. *European Food Research and Technology*, vol. 226, no. 6, pp. 1513-1524. <http://dx.doi.org/10.1007/s00217-007-0683-z>.
- BUSTIN, S.A., BENES, V., GARSON, J.A., HELLEMANS, J., HUGGETT, J., KUBISTA, M., MUELLER, R., NOLAN, T., PFAFFL, M.W., SHIPLEY, G.L., VANDESOMPELE, J. and WITWER, C.T., 2009. The MIQE guidelines: minimum information for publication of quantitative real-time PCR experiments. *Clinical Chemistry*, vol. 55, no. 4, pp. 611-622. <http://dx.doi.org/10.1373/clinchem.2008.112797>. PMID:19246619.
- CORLESS, C.E., GUIVER, M., BORROW, R., EDWARDS-JONES, V., KACZMARSKI, E.B. and FOX, A.J., 2000. Contamination and sensitivity issues with a real-time universal 16S rRNA PCR. *Journal of Clinical Microbiology*, vol. 38, no. 5, pp. 47-52. <http://dx.doi.org/10.1128/JCM.38.5.1747-1752.2000>. PMID:10790092.
- DAS, S., KALE, M., BEENA, P.M. and KUMAR, H., 2015. Bacterial contamination of platelet at University Hospital: "A prospective surveillance study. *INSS*, vol. 4, no. 4, pp. 505-508.
- DOBBELAER, I., NEERKEN, S., VAN DE WIEL, P., VAN MEERBERGEN, B., and PENTERMAN, R. *Selective lysis of cells by ionic surfactants*. n° WO2012168003 A1. 13-12-2012.
- ECKER, D.J., SAMPATH, R., LI, H., MASSIRE, C., MATTHEWS, H.E., TOLENO, D., HALL, T.A., BLYN, L.B., ESHOO, M.W., RANKEN, R., HOFSTADLER, S.A. and TANG, Y.W., 2010. New technology for rapid molecular diagnosis of bloodstream infections. *Expert Review of Molecular Diagnostics*, vol. 10, no. 4, pp. 399-415. <http://dx.doi.org/10.1586/erm.10.24>. PMID:20465496.
- ESMAILI, M.A., RAZJOU, F., KHOSROSHAHI, B.N., et al. 2017. Evaluations of detections methods of bacterial contamination in platelet components. *International Journal of Medical Laboratory*, vol. 4, no. 4, pp. 232-245.
- EZUKI, S., KAWABATA, K., KANNO, T. and OHTO, H., 2007. Culture-based bacterial detection systems for platelets: the effect of time prior to sampling and duration of incubation required for detection with aerobic culture. *Transfusion*, vol. 47, no. 11, pp. 2044-2049. <http://dx.doi.org/10.1111/j.1537-2995.2007.01428.x>. PMID:17958533.
- FISHER, R.A., 1956. *Statistical methods for research workers*. 12th ed. London: Quarterly Journal of the Royal Meteorol Society.

- GARSON, J.A., PATEL, P., MCDONALD, C., BALL, J., ROSENBERG, G., TETTMAR, K.I., BRAILSFORD, S.R., PITT, T. and TEDDER, R.S. 2014. Evaluation of an ethidium monoazide-enhanced 16S rDNA real-time polymerase chain reaction assay for bacterial screening of platelet concentrates and comparison with automated culture. *Transfusion*, vol. 54, no. 3 Pt 2, pp. 870-878. <http://dx.doi.org/10.1111/trf.12256>. PMID:23701338.
- HEIN, I., SCHNEEWEISS, W., STANEK, C. and WAGNER, M., 2007. Ethidium monoazide and propidium monoazide for elimination of unspecific DNA background in quantitative universal real-time PCR. *Journal of Microbiological Methods*, vol. 71, no. 3, pp. 336-339. <http://dx.doi.org/10.1016/j.mimet.2007.09.005>. PMID:17936386.
- HENDOLIN, P.H., MARKKANEN, A., YLIKOSKI, J. and WAHLFORS, J.J., 1997. Use of multiplex PCR for simultaneous detection of four bacterial species in middle ear effusions. *Journal of Clinical Microbiology*, vol. 35, no. 11, pp. 2854-2858. <http://dx.doi.org/10.1128/JCM.35.11.2854-2858.1997>. PMID:9350746.
- HUMPHREY, B., MCLEOD, N., TURNER, C., SUTTON, J.M., DARK, P.M. and WARHURST, G., 2015. Removal of contaminant DNA by combined UV-EMA treatment allows low copy number detection of clinically relevant bacteria using pan-bacterial real-time PCR. *PLoS One*, vol. 10, no. 7, pp. e0132954. <http://dx.doi.org/10.1371/journal.pone.0132954>. PMID:26172943.
- KLAUSEGGER, A., HELL, M., BERGER, A., ZINOBER, K., BAIER, S., JONES, N., SPERL, W. and KOFLER, B., 1999. Gram type-specific broad-range PCR amplification for rapid detection of 62 pathogenic bacteria. *Journal of Clinical Microbiology*, vol. 37, no. 2, pp. 464-466. <http://dx.doi.org/10.1128/JCM.37.2.464-466.1999>. PMID:9889245.
- KUMAR, S., STECHER, G. and TAMURA, K., 2016. MEGA 7: Molecular evolutionary genetics analysis version 7.0 for bigger datasets. *Molecular Biology and Evolution*, vol. 33, no. 7, pp. 1870-1874. <http://dx.doi.org/10.1093/molbev/msw054>. PMID:27004904.
- LOONEN, A. J. M., BOS, M. P., VAN MEERBERGEN, B., NEERKEN, S., CATSBURG, A., DOBBELAER, I., PENTERMAN, R., MAERTENS, G., VAN DE WIEL, P., SAVELKOUL, P., and VAN DEN BRULE, A. J. C., 2013. Comparison of pathogen DNA isolation methods from large volumes of whole blood to improve molecular diagnosis of bloodstream infections. *Plos One*, vol. 8, no. 8, pp. e72349.
- MACAULEY, A., CHANDRASEKAR, A., GEDDIS, G., MORRIS, K.G. and MCCLELLAND, W.M., 2003. Operational feasibility of routine bacterial monitoring of platelets. *Transfusion Medicine (Oxford, England)*, vol. 13, no. 4, pp. 189-195. <http://dx.doi.org/10.1046/j.1365-3148.2003.00441.x>. PMID:12880389.
- MANCINI, N., CARLETTI, S., GHIDOLI, N., CICHERO, P., BURIONI, R. and CLEMENTI, M., 2010. The era of molecular and other non-culture based methods in diagnosis of sepsis. *Clinical Microbiology Reviews*, vol. 23, no. 1, pp. 235-251. <http://dx.doi.org/10.1128/CMR.00043-09>. PMID:20065332.
- MOHAMMADI, T., PIETERSZ, R.N., VANDENBROUCKE-GRAULS, C.M., SAVELKOUL, P.H. and REESINK, H.W., 2005. Detection of bacteria in platelet concentrates: comparison of broad-range real-time 16S rDNA polymerase chain reaction and automated culturing. *Transfusion*, vol. 45, no. 5, pp. 731-736. <http://dx.doi.org/10.1111/j.1537-2995.2005.04258.x>. PMID:15847662.
- MOHAMMADI, T., SAVELKOUL, P.H., PIETERSZ, R.N. and REESINK, H.W., 2006. Applications of real-time PCR in the screening of platelet concentrates for bacterial contamination. *Expert Review of Molecular Diagnostics*, vol. 6, no. 6, pp. 865-872. <http://dx.doi.org/10.1586/14737159.6.6.865>. PMID:17140373.
- PALAVECINO, E. and YOMTOVIAN, R., 2003. Risk and prevention of transfusion-related sepsis. *Current Opinion in Hematology*, vol. 10, no. 6, pp. 434-439. <http://dx.doi.org/10.1097/00062752-200311000-00007>. PMID:14564174.
- PALAVECINO, E.L., YOMTOVIAN, R.A. and JACOBS, M.R., 2006. Detecting bacterial contamination in platelet products. *Clinical Laboratory*, vol. 56, no. 9-10, pp. 443-456. PMID:17078471.
- PAOLUCCI, M., LANDINI, M.P. and SAMBRI, V., 2010. Conventional and molecular techniques for the early diagnosis of bacteraemia. *International Journal of Antimicrobial Agents*, vol. 36, suppl. 2, pp. S6-S16. <http://dx.doi.org/10.1016/j.ijantimicag.2010.11.010>. PMID:21129933.
- PATEL, P., GARSON, J.A., TETTMAR, K.I., ANCLIFF, S., MCDONALD, C., PITT, T., COELHO, J. and TEDDER, R.S., 2012. Development of an ethidium monoazide-enhanced internally controlled universal 16S rDNA real-time polymerase chain reaction assay for detection of bacterial contamination in platelet concentrates. *Transfusion*, vol. 52, no. 7, pp. 1423-1432. <http://dx.doi.org/10.1111/j.1537-2995.2011.03484.x>. PMID:22188457.
- PIETERSZ, R.N., ENGELFRIET, C.P. and REESINK, H.W., 2003. Detection of bacterial contamination of platelet concentrates. *Vox Sanguinis*, vol. 85, no. 3, pp. 224-239. PMID:14516456.
- RAZJOU, F., NAGHADEH, H.T., FERDOWSI, S. and DABIRMOGHADAM, A., 2017. Evaluation of the sensitivity and specificity of use of glucose and pH for bacterial screening of platelet concentrates compared to the Bact/Alert. *Indian Journal of Hematology & Blood Transfusion : An Official Journal of Indian Society of Hematology and Blood Transfusion*, vol. 33, no. 1, pp. 116-120. <http://dx.doi.org/10.1007/s12288-016-0660-4>. PMID:28194067.
- ROOD, I.G., PETERSSON, A., SAVELKOUL, P.H. and DE KORTE, D., 2011. Performance and suitability of polymerase chain reaction for early detection of bacteria in platelet concentrates. *Transfusion*, vol. 51, no. 9, pp. 2006-2011. <http://dx.doi.org/10.1111/j.1537-2995.2011.03090.x>. PMID:21392020.
- RUECKERT, A. and MORGAN, H.W., 2007. Removal of contaminating DNA from polymerase chain reaction using ethidium monoazide. *Journal of Microbiological Methods*, vol. 68, no. 3, pp. 596-600. <http://dx.doi.org/10.1016/j.mimet.2006.11.006>. PMID:17187883.
- SCHREZENMEIER, H., WALTHER-WENKE, G., MULLER, T.H., WEINAUER, F., YOUNIS, A., HOLLAND-LETZ, T., GEIS, G., ASMUS, J., BAUERFEIND, U., BURKHART, J., DEITENBECK, R., FÖRSTEMANN, E., GEBAUER, W., HÖCHSMANN, B., KARAKASSOPOULOS, A., LIEBSCHER, U.M., SÄNGER, W., SCHMIDT, M., SCHUNTER, F., SIREIS, W. and SEIFRIED, E., 2007. Bacterial contamination of platelet concentrates: results of a prospective multicenter study comparing pooled whole blood-derived platelets and apheresis platelets. *Transfusion*, vol. 47, no. 4, pp. 644-652. <http://dx.doi.org/10.1111/j.1537-2995.2007.01166.x>. PMID:17381623.
- TAKAHASHI, H., YAMAZAKI, H., AKANUMA, S., KANAHARA, H., SAITO, T., CHIMURO, T., KOBAYASHI, T., OHTANI, T., YAMAMOTO, K., SUGIYAMA, S. and KOBORI, T., 2014. Preparation of Phi29 DNA Polymerase free of Amplifiable DNA using Ethidium Monoazide, an ultraviolet-free light-emitting diode lamp and trehalose. *PLoS One*, vol. 9, no.

2, pp. e82624. <http://dx.doi.org/10.1371/journal.pone.0082624>. PMID:24505243.

TRUNG, N.T., HIEN, T.T.T., HUYEN, T.T.T., QUYEN, D.T., VAN SON, T., HOAN, P.Q., PHUONG, N.T., LIEN, T.T., BINH, M.T., VAN TONG, H., MEYER, C.G., VELAVAN, T.P. and SONG, H., 2016. Enrichment of bacterial DNA for the diagnosis of blood stream infections. *BMC Infectious Diseases*, vol. 16, no. 1, pp. 235. <http://dx.doi.org/10.1186/s12879-016-1568-1>. PMID:27246723.

VAN MEERBERGEN, B.E.G.J., PICIU, O.M., GIL, R., SCHMIDT, K.A., NEERKEN, S., PONJEE, M.W.G., UNAY, Z.S., PENTERMAN, R. and VAN DE WIEL, P.A. *Selective lysis of cell*. n° WO2011070507 A1. 16-06-2011.

WAGNER, S.J., 2004. Transfusion-transmitted bacterial infection: Risks, sources and interventions. *Vox Sanguinis*, vol. 86, no. 3, pp. 157-163. <http://dx.doi.org/10.1111/j.0042-9007.2004.00410.x>. PMID:15078249.

WALTHER-WENKE, G., 2008. Incidence of bacterial transmission and transfusion reactions by blood components. *Clinical Chemistry*

*and Laboratory Medicine*, vol. 46, no. 7, pp. 919-925. <http://dx.doi.org/10.1515/CCLM.2008.151>. PMID:18605950.

WILSON, K.H., BLITCHINGTON, R.B. and GREENE, R.C., 1990. Amplification of bacterial 16S ribosomal DNA with polymerase chain reaction. *Journal of Clinical Microbiology*, vol. 28, no. 9, pp. 1942-1946. <http://dx.doi.org/10.1128/JCM.28.9.1942-1946.1990>. PMID:2095137.

WORLD HEALTH ORGANIZATION – WHO, 2009. *CDC protocol of real time RT-PCR for swine influenza A(H1N1)*. Geneva: WHO, pp. 1-9.

YANG, S., LIN, S., KELEN, G.D., QUINN, T.C., DICK, J.D., GAYDOS, C.A. and ROTHMAN, R.E., 2002. Quantitative multiprobe PCR assay for simultaneous detection and identification to species level of bacterial pathogens. *Journal of Clinical Microbiology*, vol. 40, no. 9, pp. 3449-3454. <http://dx.doi.org/10.1128/JCM.40.9.3449-3454.2002>. PMID:12202592.